

CALIBRATOR
James R. Braig, et al.
Appl. No.: Unknown Atty Docket: OPTIS.010DVI

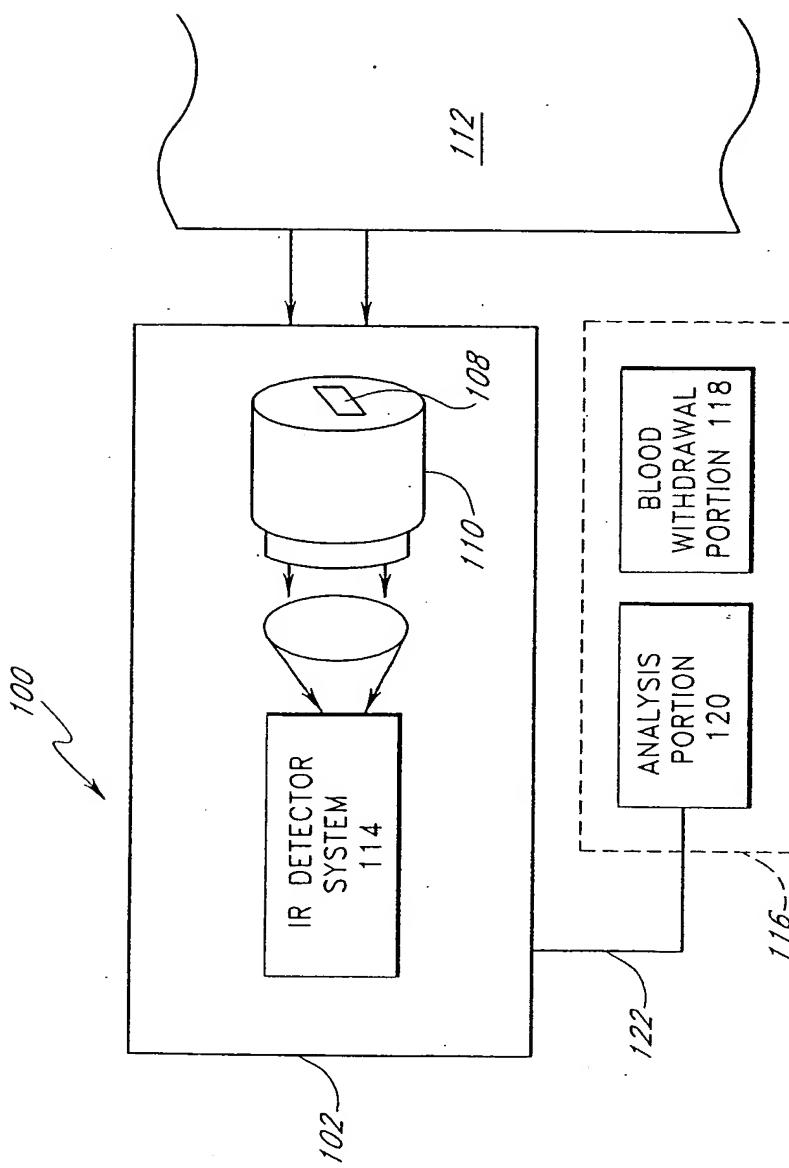


FIG. 1

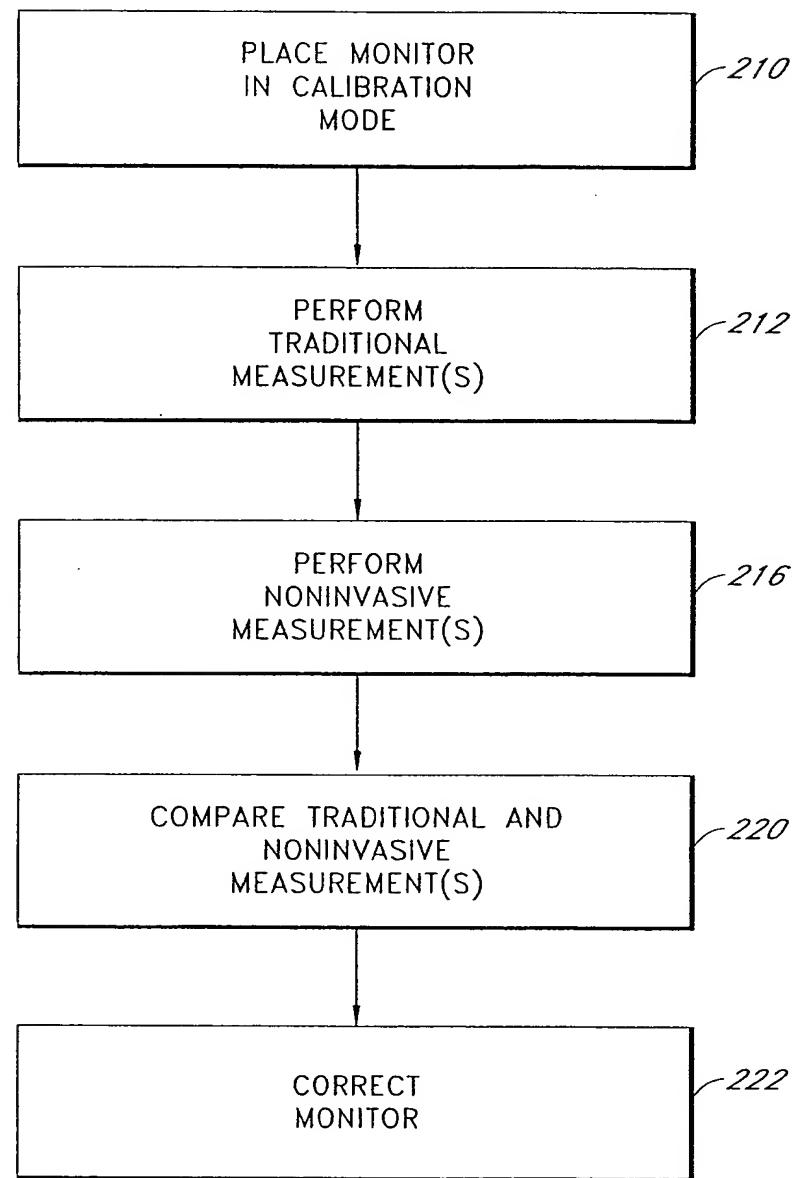


FIG. 2

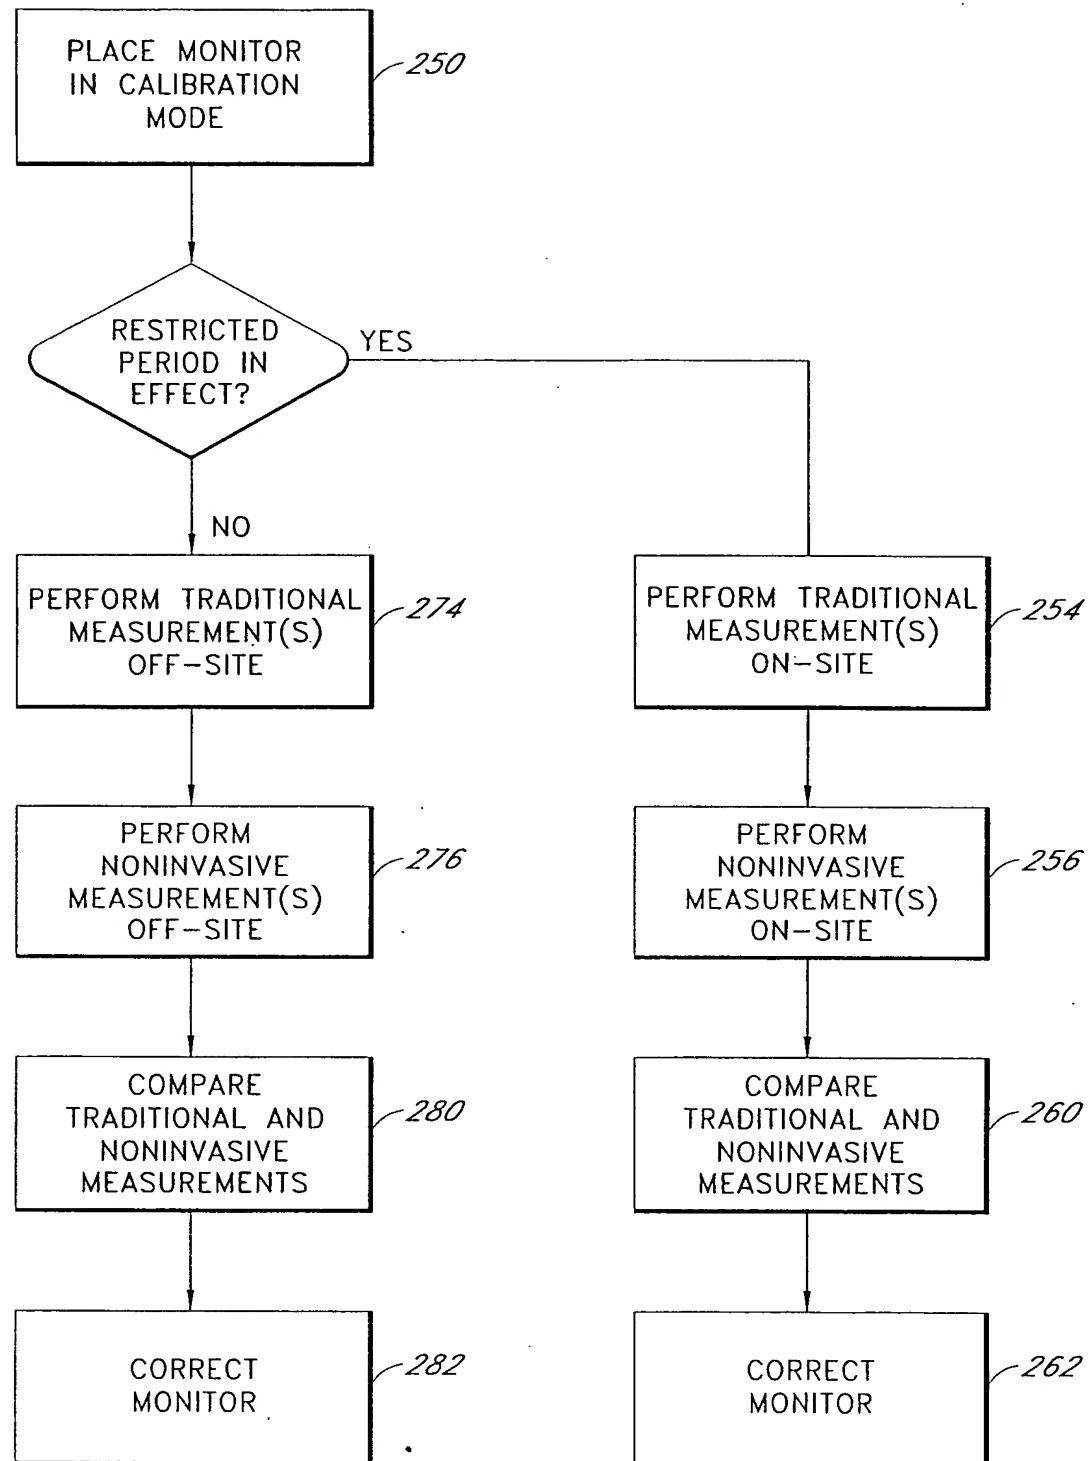


FIG. 2A

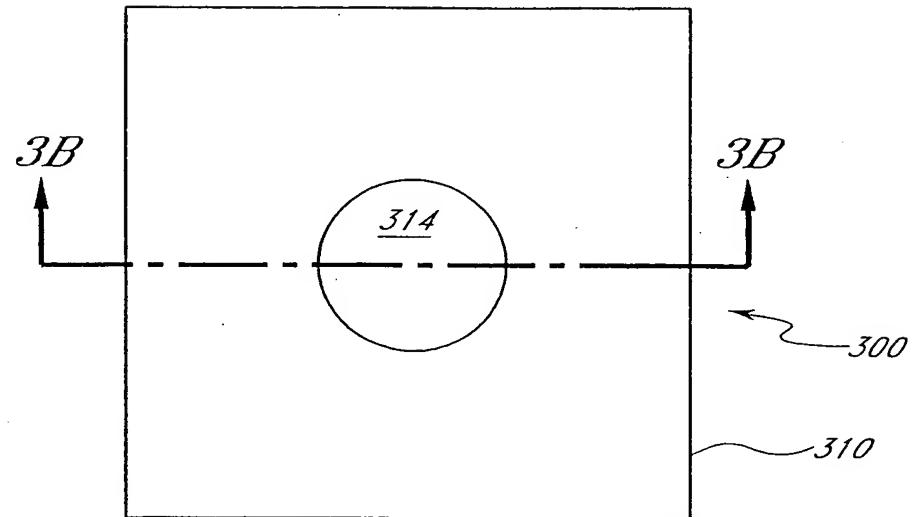


FIG. 3A

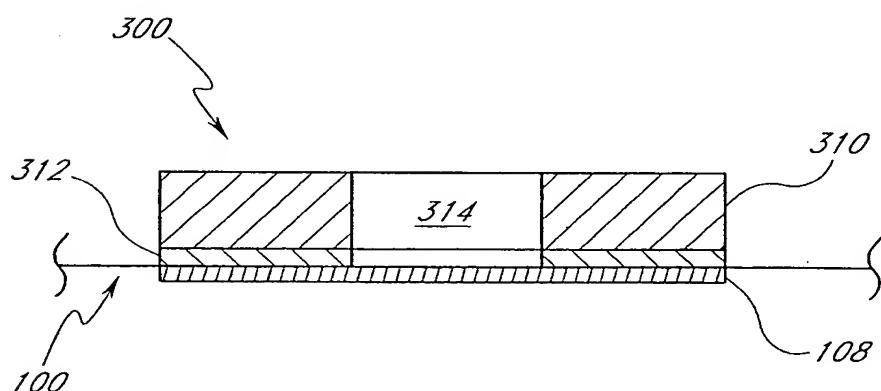


FIG. 3B

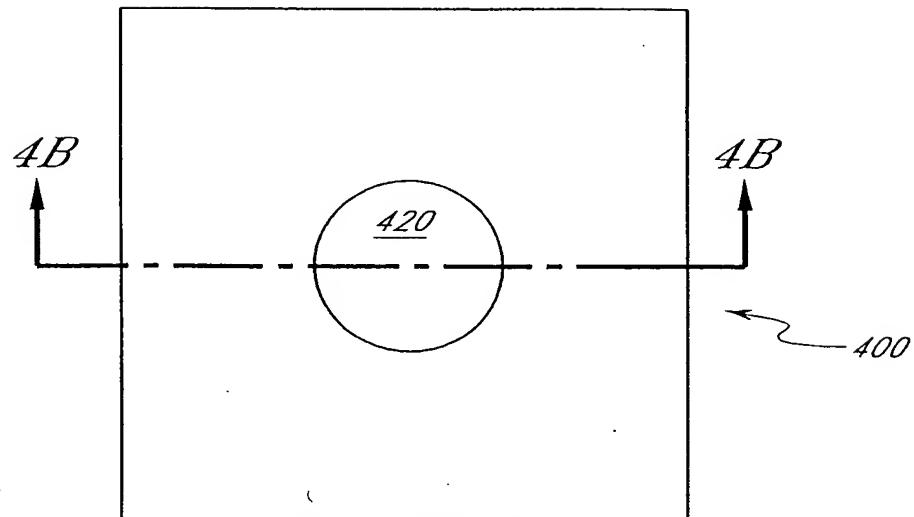


FIG. 4A

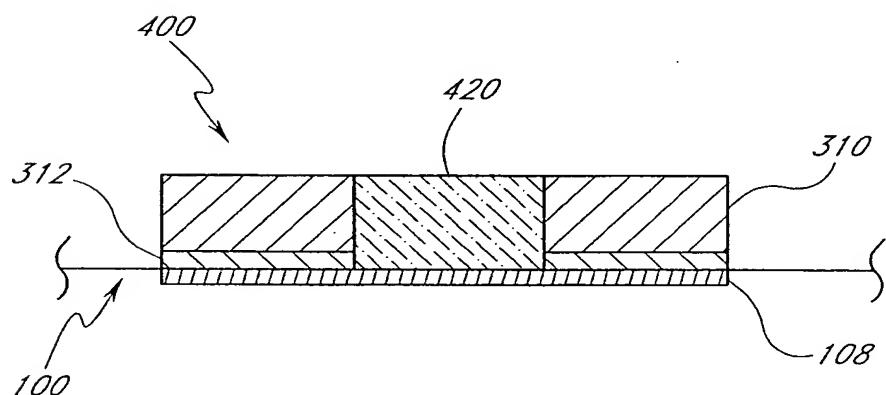


FIG. 4B

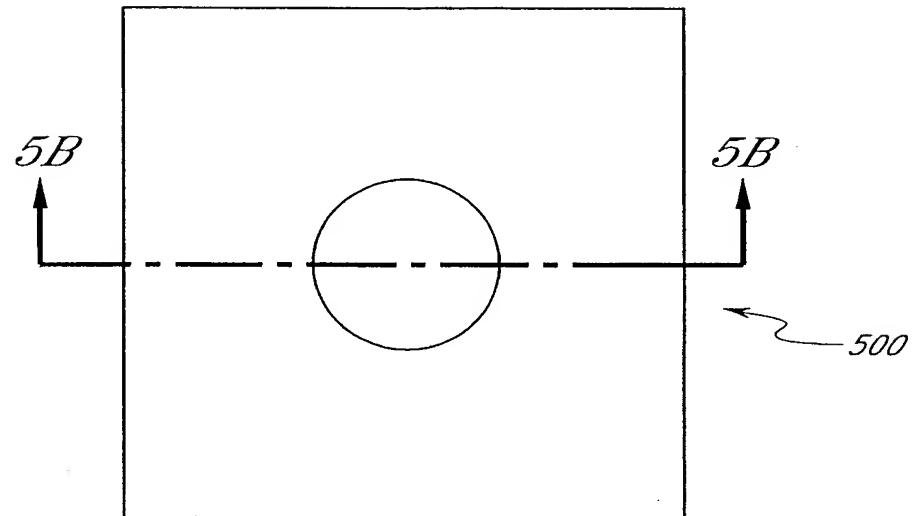


FIG. 5A

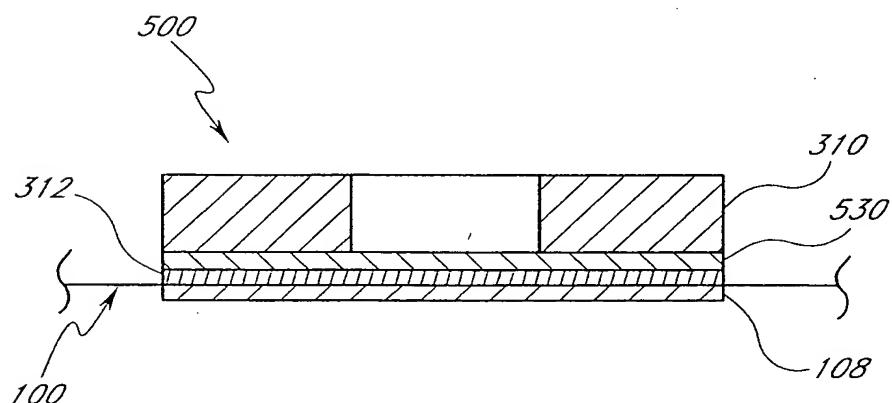


FIG. 5B

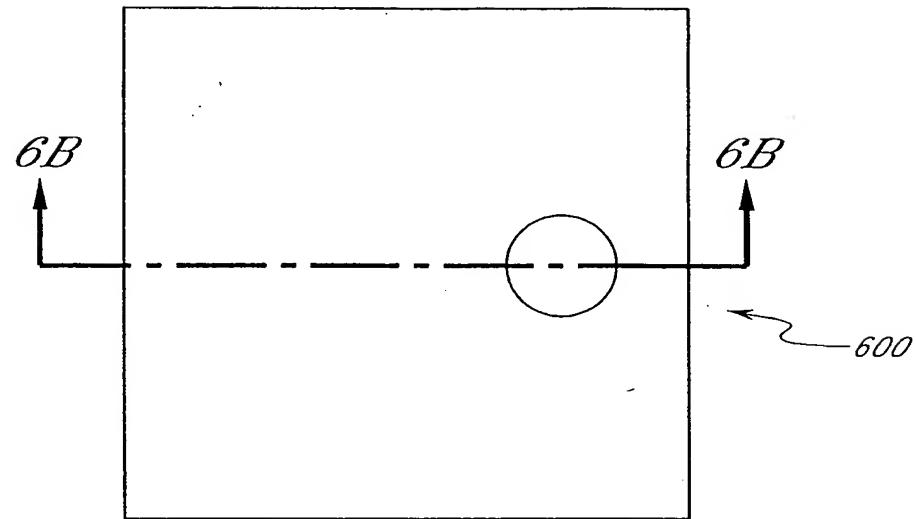


FIG. 6A

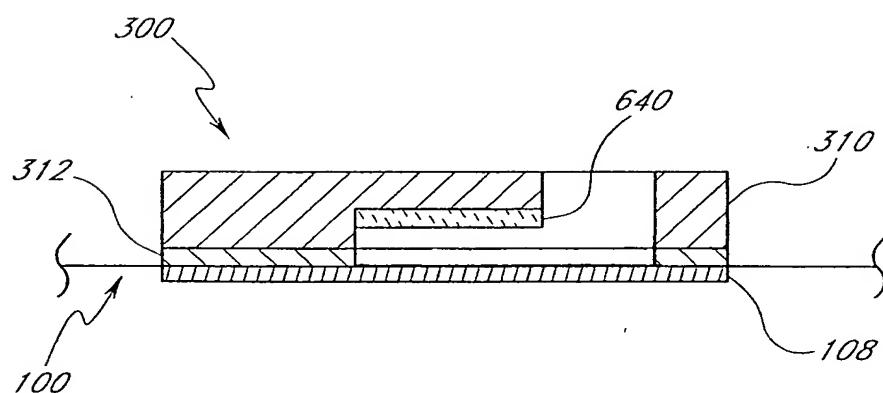


FIG. 6B